

100

FIGURE 1 A

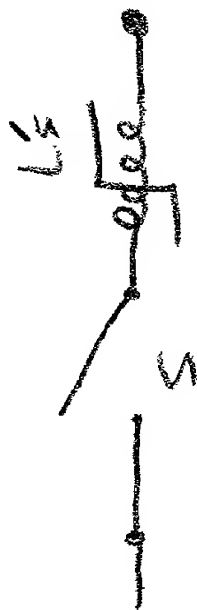


Figure 1c

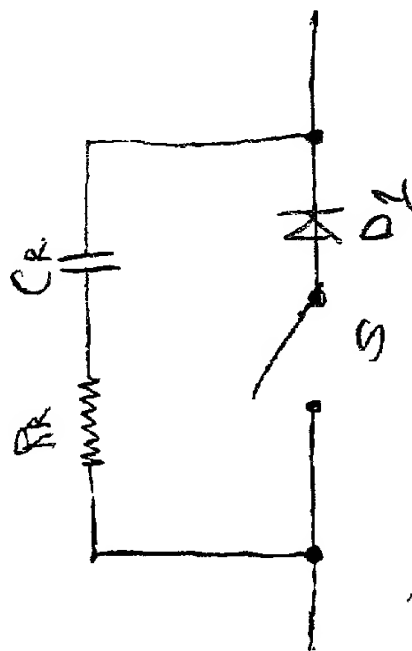


Figure 1B

FIG. 1A

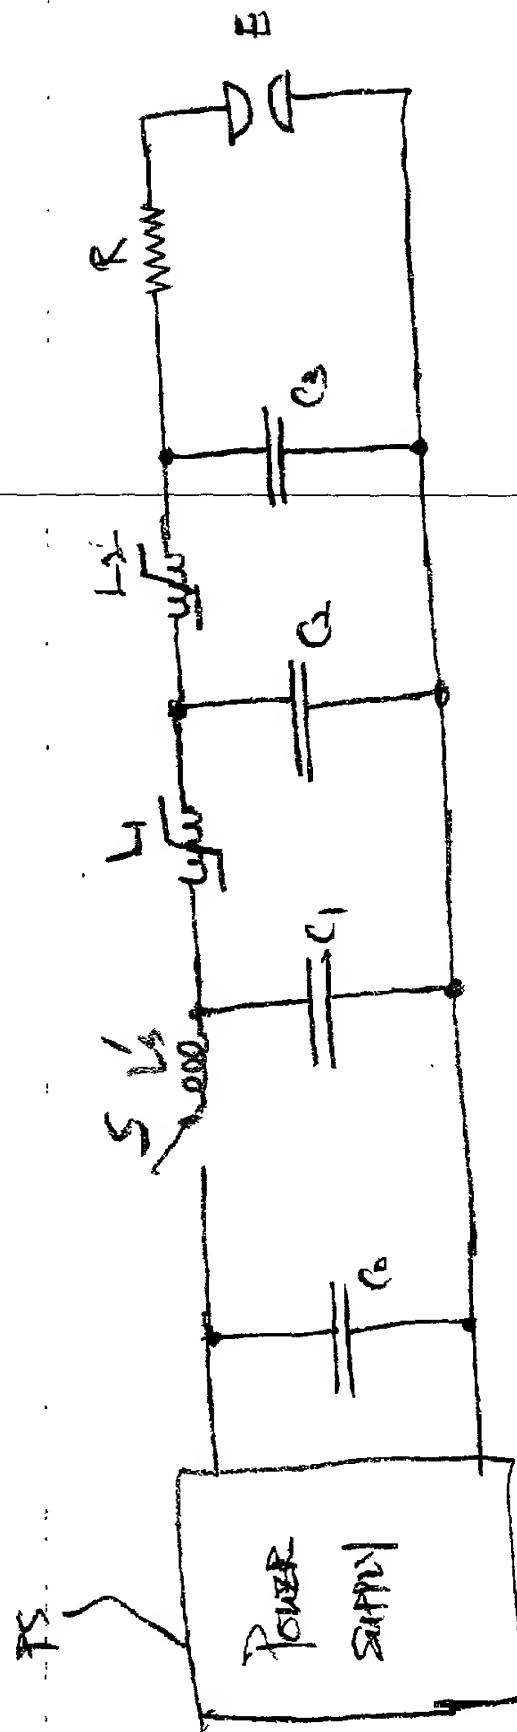


FIGURE 2A

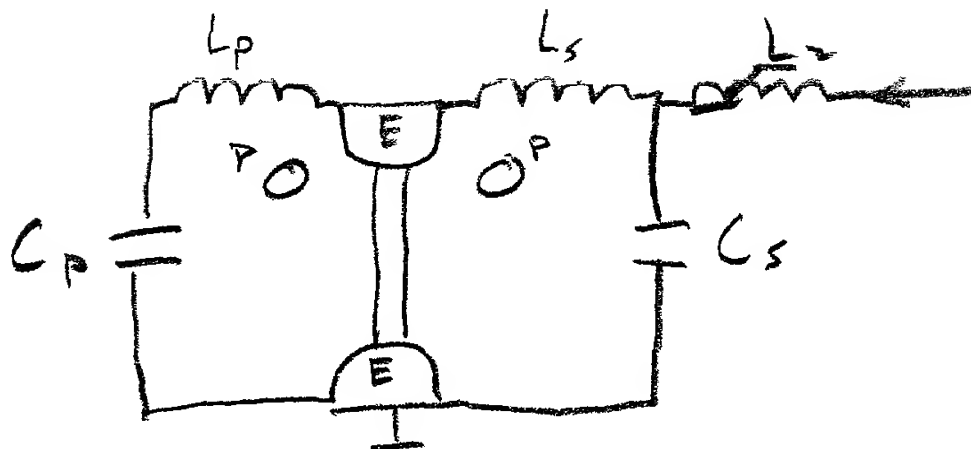


Figure 2B

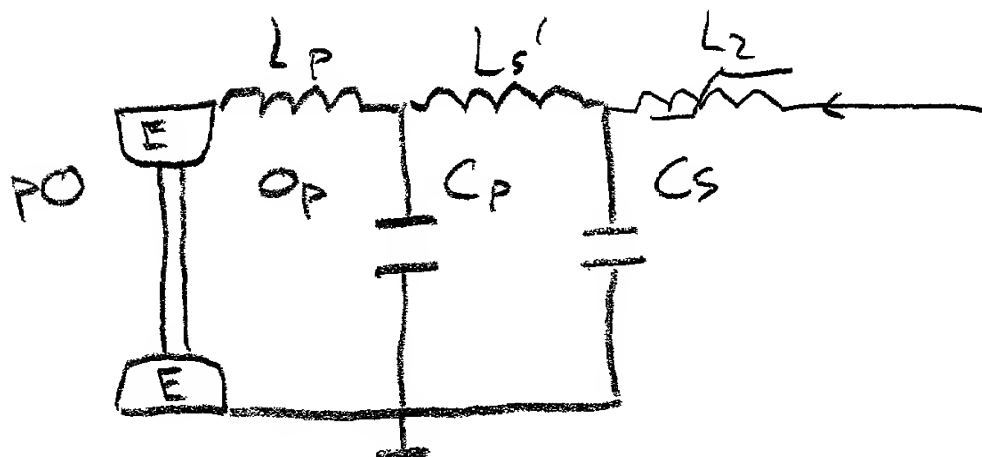


Figure 2C

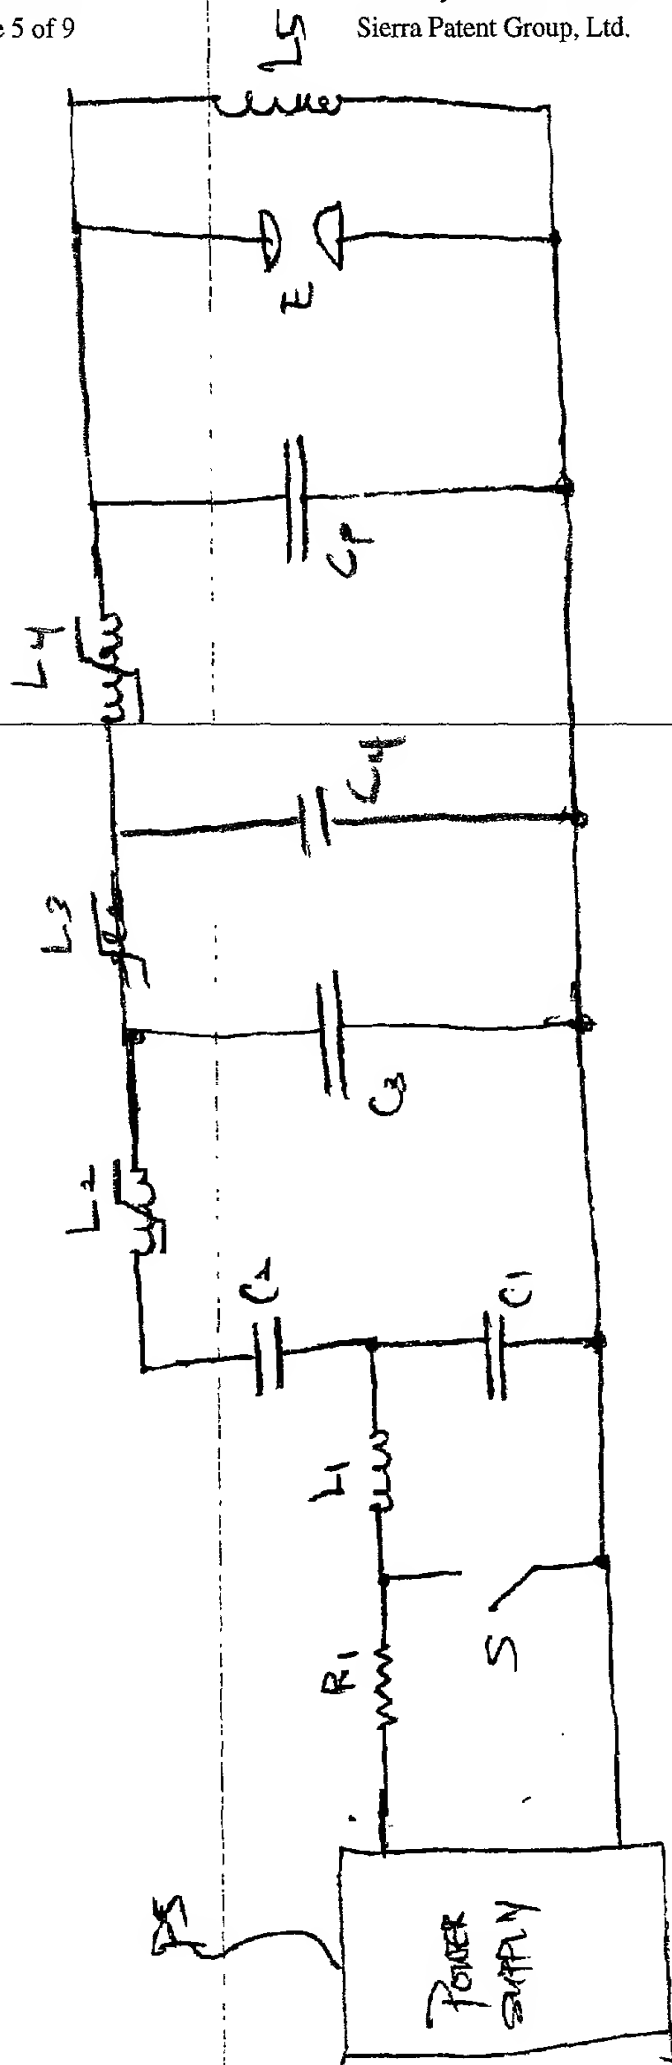


FIGURE 3

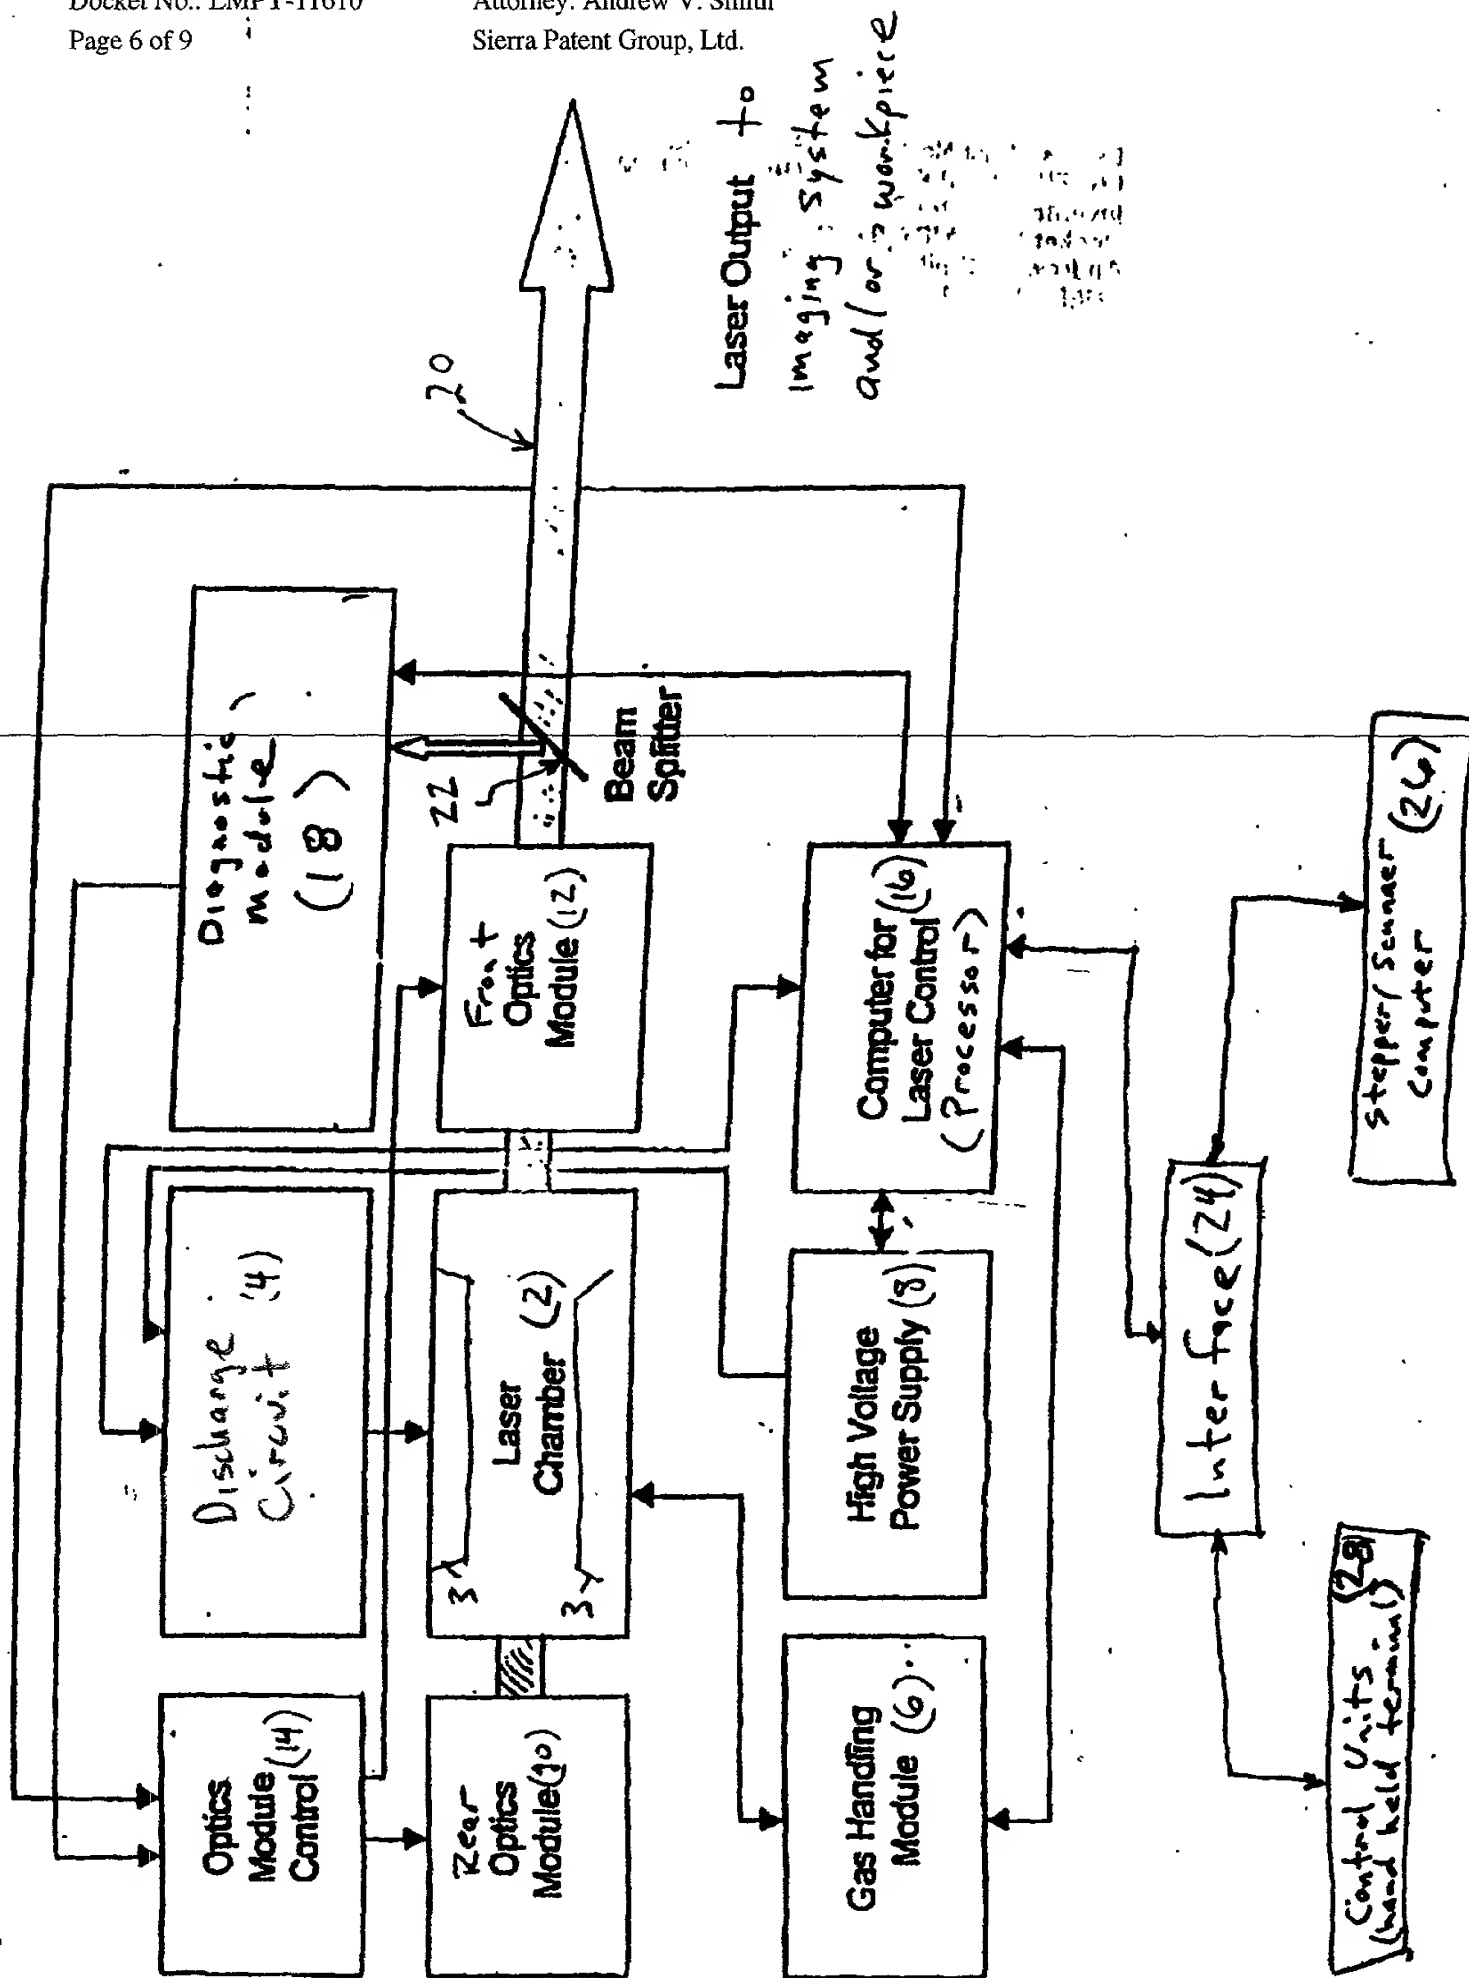
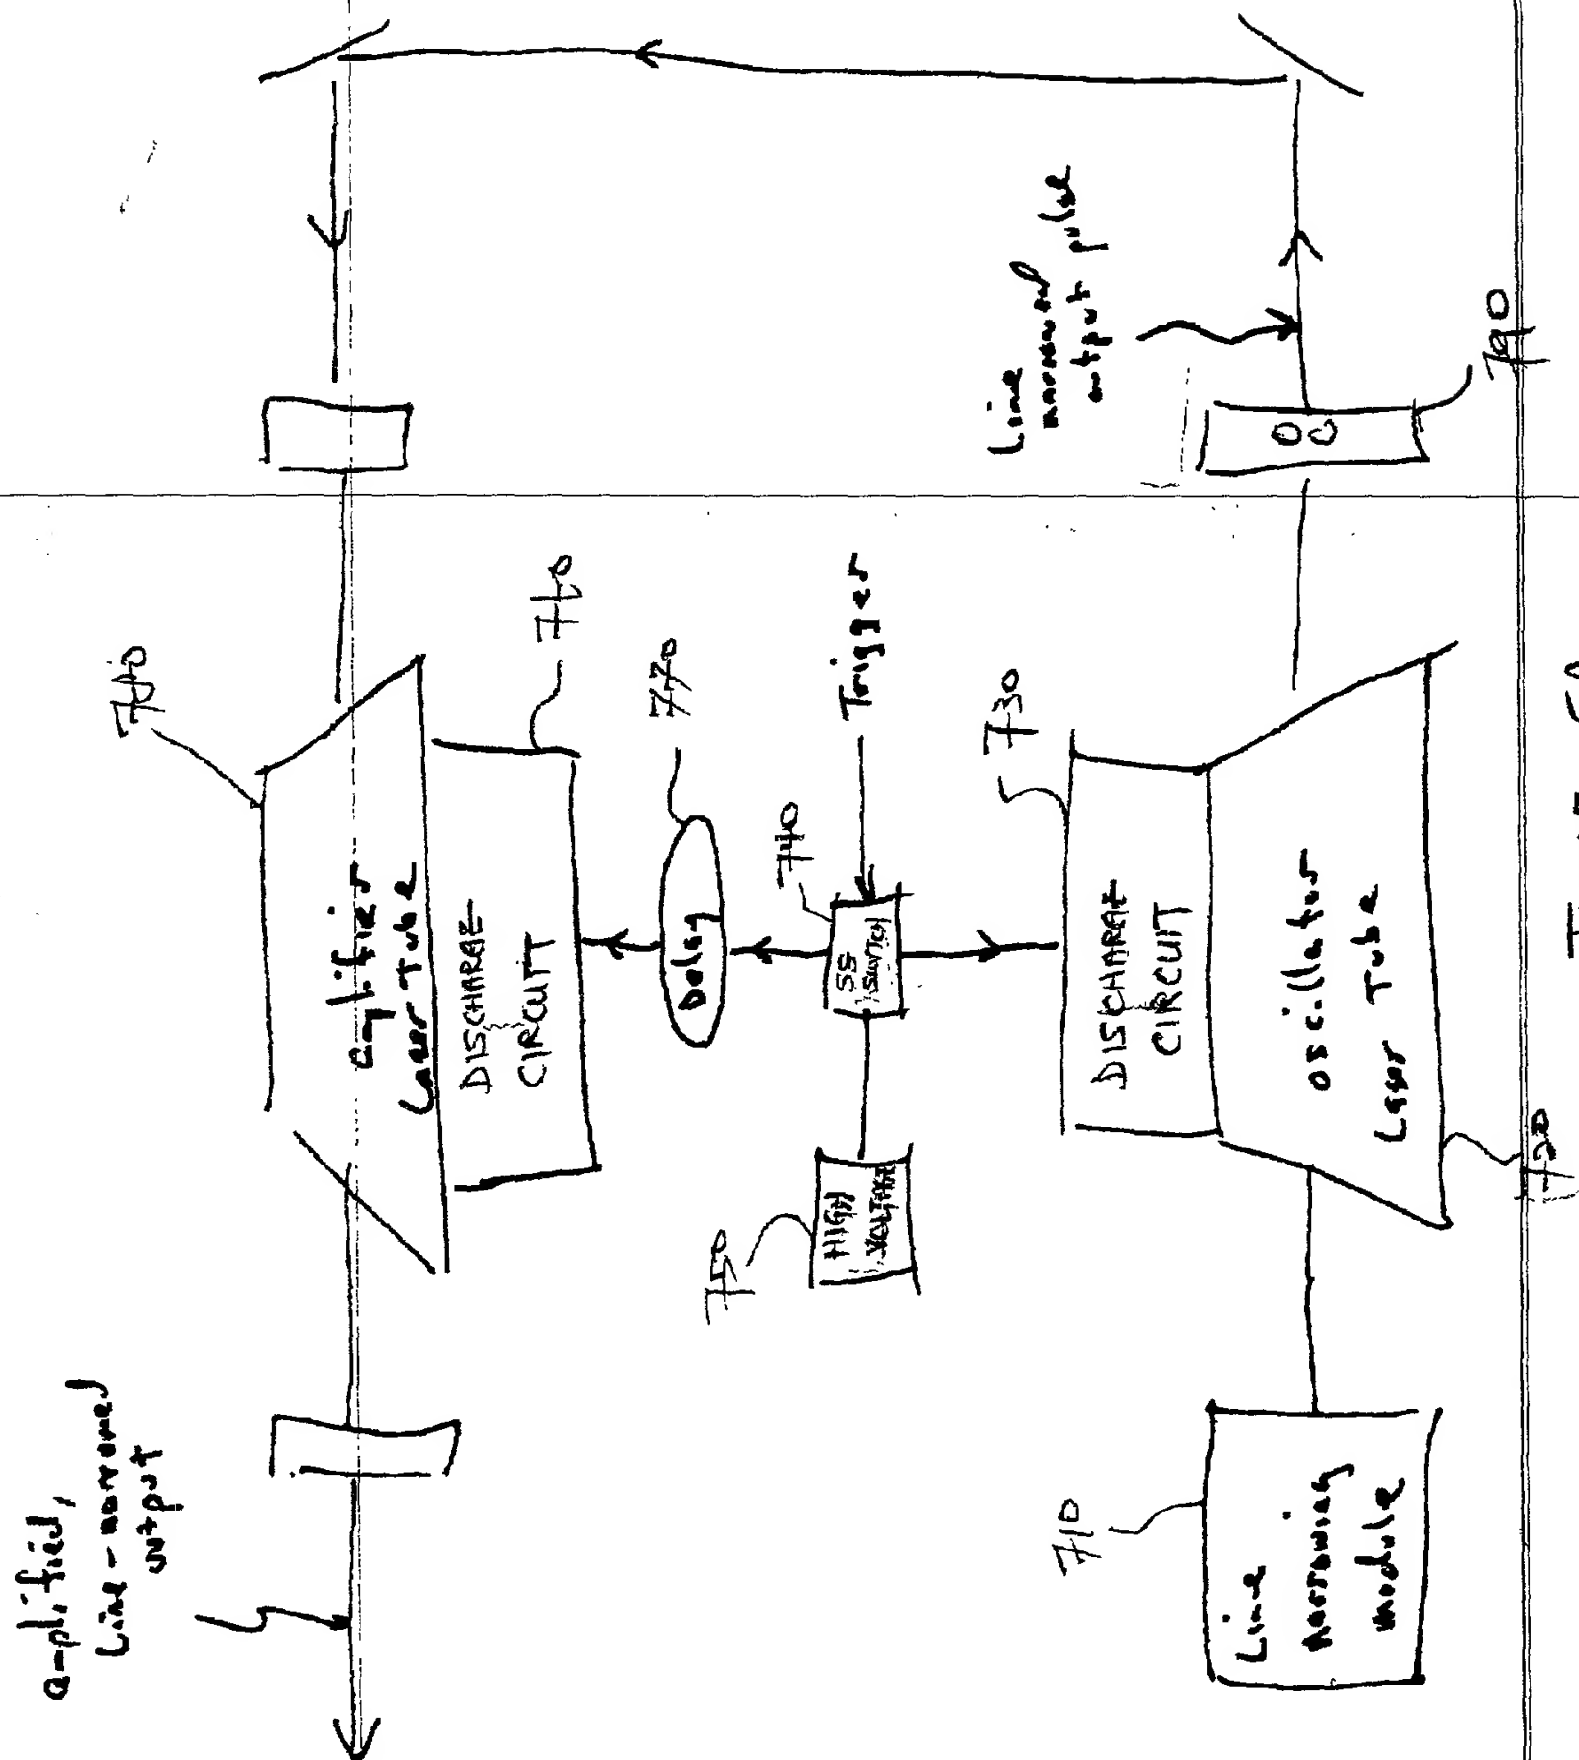


Figure 4





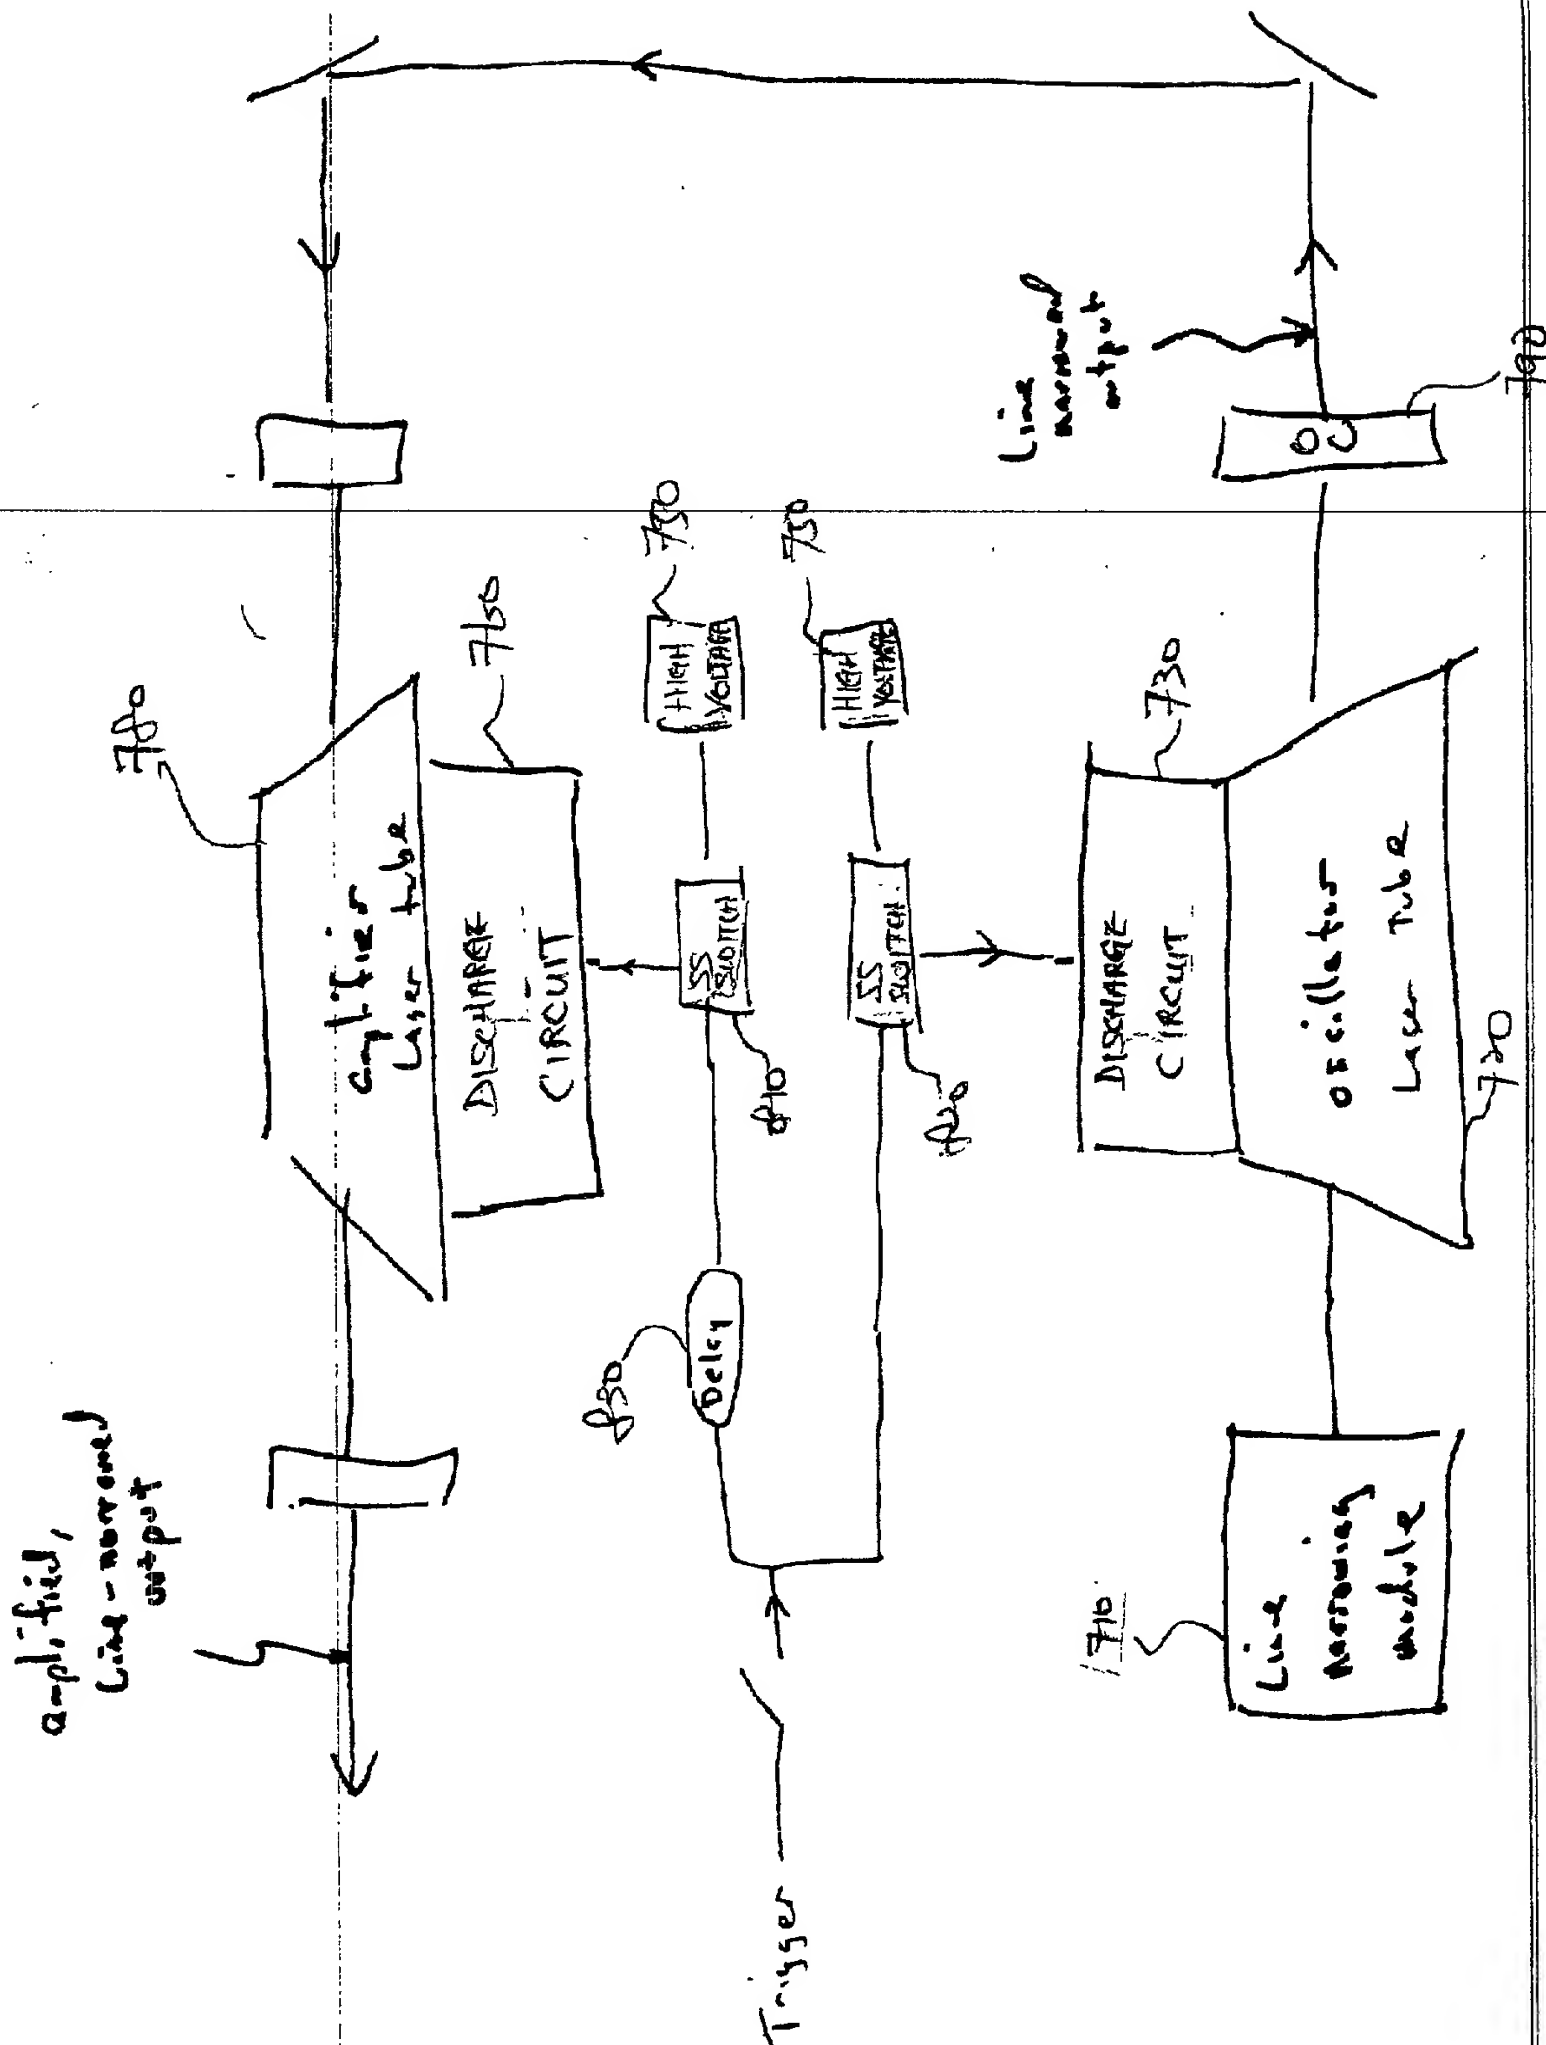


FIGURE 5B

L_4308 B+ , E 5153, tube 473k, 1 x EMI, Run test with SSW

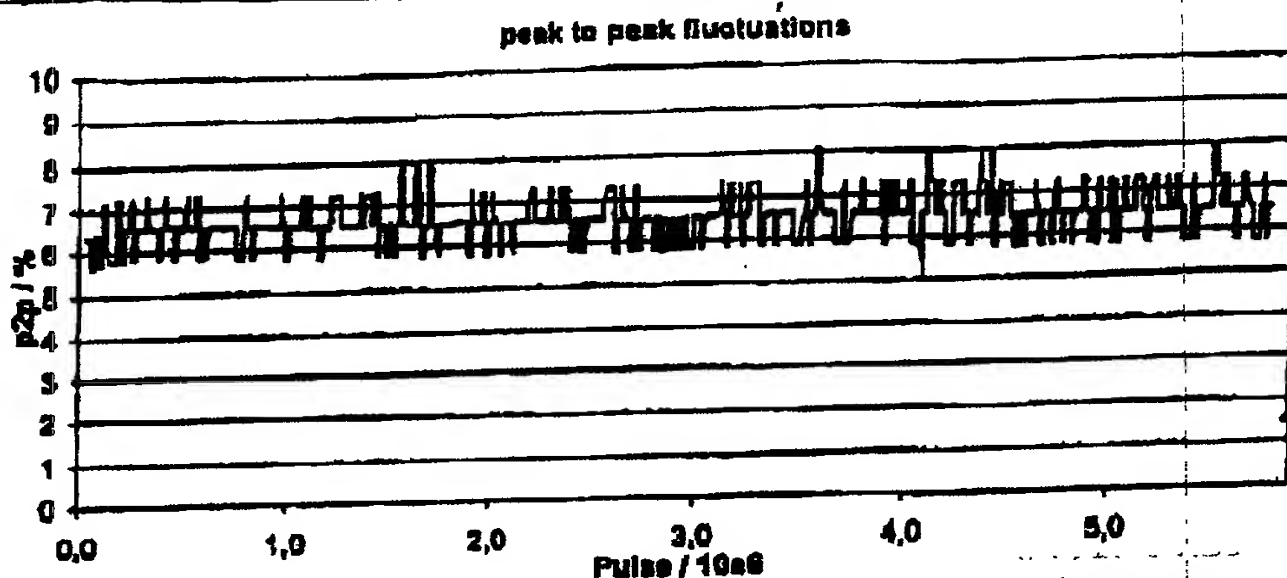

average (p2p) = 6.66 3 Pulses in 382 measured intervals or 0.8 % are above 8 %
 sigma (average (p2p)) = 0.61 304 Pulses in 382 measured intervals or 79.6 % are above 6 %
 382 Pulses in 382 measured intervals or 100 % are above 4 %

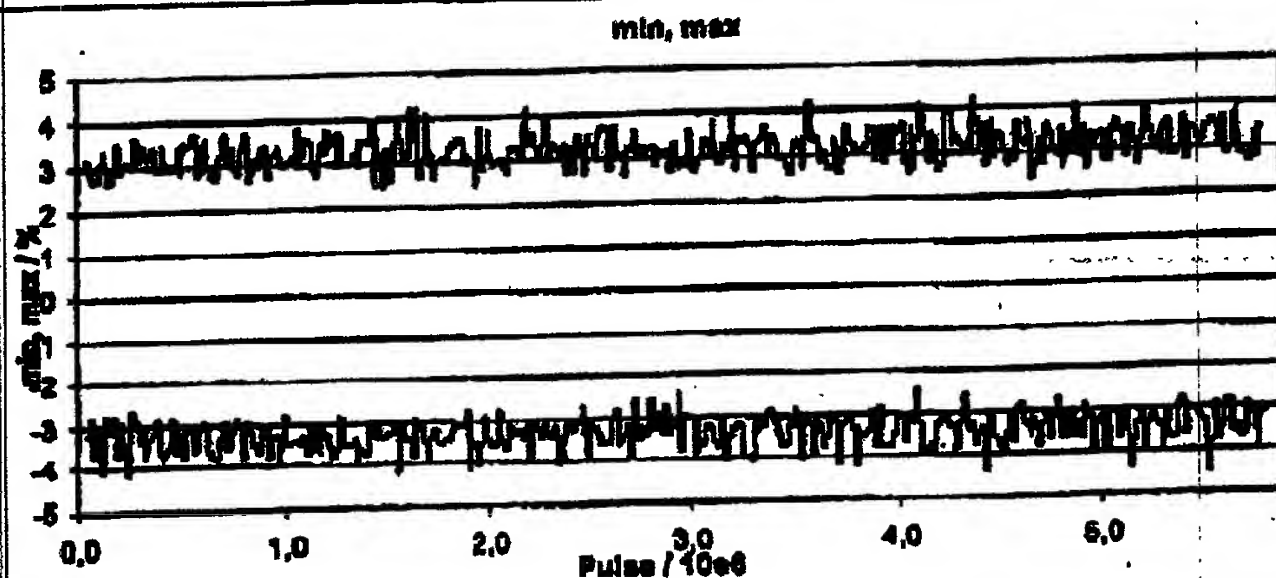

average (min) = -3.35 17 Pulses in 382 measured intervals or 4.5 % are below -4 %
 sigma (average (min)) = 0.98 332 Pulses in 382 measured intervals or 86.9 % are below -3 %
 382 Pulses in 382 measured intervals or 100 % are below -2 %
 average (max) = 3.21 382 Pulses in 382 measured intervals or 100 % are above 2 %
 sigma (average (max)) = 0.34 288 Pulses in 382 measured intervals or 75.2 % are above 3 %
 8 Pulses in 382 measured intervals or 2.1 % are above 4 %

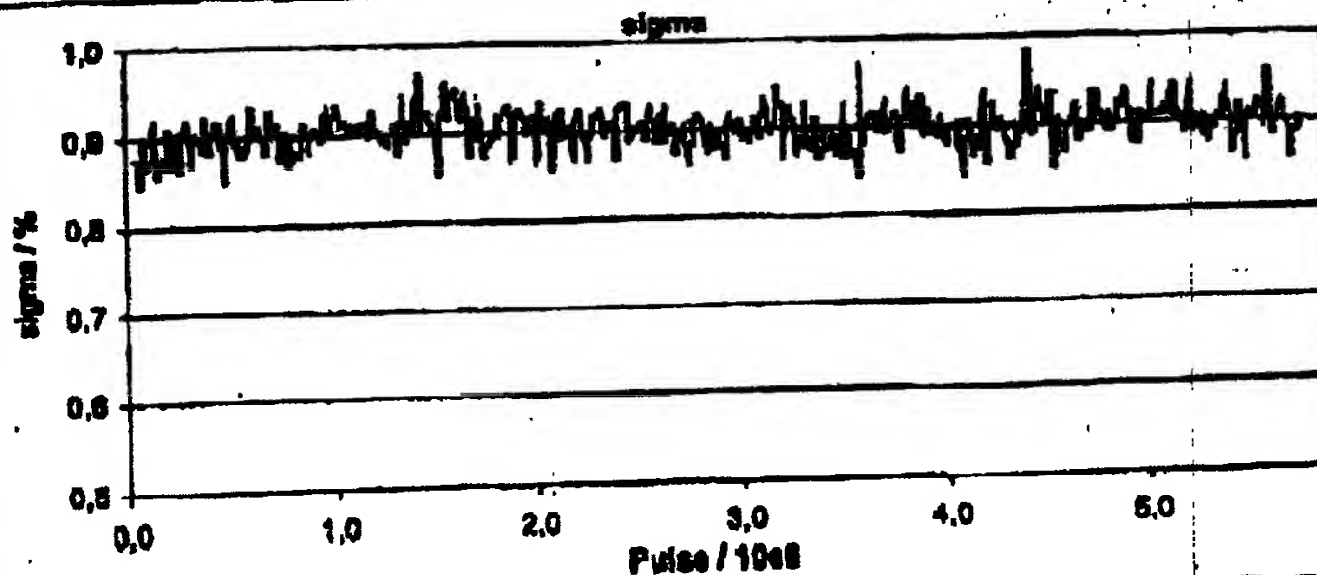


FIGURE 6A

FIGURE 6B

FIGURE 6C